


Instruction Manual

HI 93740 Nickel Low Range ISM

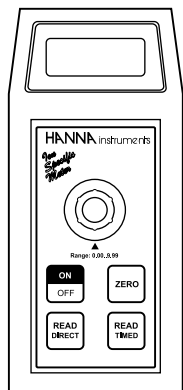

WARRANTY

HI 93740 is warranted for two years against defects in workmanship and materials when used for its intended purpose and maintained according to instructions.

This warranty is limited to repair or replacement free of charge.

Damages due to accident, misuse, tampering or lack of prescribed maintenance are not covered.

If service is required, contact the dealer from whom you purchased the instrument. If under warranty, report the model number, date of purchase, serial number and the nature of the failure. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the instrument is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization Number from the Customer Service department and then send it with shipment costs prepaid. When shipping any instrument, make sure it is properly packaged for complete protection.

To validate your warranty, fill out and return the enclosed warranty card within 14 days from the date of purchase.

All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA.

Hanna Instruments reserves the right to modify the design, construction and appearance of its products without advance notice.

Dear Customer,

Thank you for choosing a Hanna product. This manual will provide you with the necessary information for the correct operation of the meter. Please read it carefully before using the meter. If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com.

This instrument is in compliance with CE directives EN 50081-1 and EN 50082-1.

PRELIMINARY EXAMINATION

Remove the instrument from the packing material and examine it carefully to make sure that no damage has occurred during shipment. If there is any damage, notify your Dealer.

Each Ion Specific Meter is supplied complete with

- 9V Battery
- Two Sample Cuvets and Caps
- One Transport Cap

Note: Conserve all packing material until the instrument has been observed to function correctly. Any defective item must be returned in its original packing.

The HI 93740 meter measures the nickel content in water and wastewater in the 0.000 to 1.000 mg/L (ppm) range.


The meter uses an exclusive positive-locking system to ensure that the cuvet is in the same place every time it is placed into the measurement cell.

The reagents are in liquid and powder form and are supplied in bottles and in packets. The amount of reagent is precisely dosed to ensure maximum repeatability.

Display codes aid the user in routine operations.

The meters have an auto-shut off feature that will turn the instrument off after 10 minutes of non-use.

SPECIFICATIONS

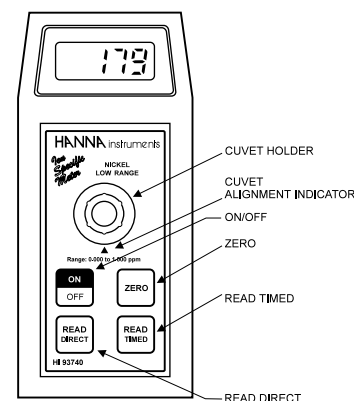

SPECIFICATIONS

Range	0.000 to 1.000 mg/L
Resolution	0.001 mg/L
Accuracy	±0.01 mg/L ±7% of reading
Typical EMC Deviation	±0.001 mg/L
Light Source	Light Emitting Diode @ 555 nm
Method	Adaptation of the 1-(2-pyridylazo)-2-naphtol (PAN) method. The reaction between nickel and the reagent causes an orange tint in the sample
Light Detector	Silicon Photocell
Environment	0 to 50°C (32 to 122°F); max 95% RH non-condensing
Battery Type/Life	1 x 9 volt/40 hours
Auto-Shut off	After 10' of non-use
Dimensions	180 x 83 x 46 mm (7.1 x 3.3 x 1.8")
Weight	290 g (10 oz.).

REQUIRED REAGENTS

Code	Description	Quantity
HI 93740A-0	Phthalate phosphate	2 packets
HI 93740B-0	0.3% PAN indicator	2 mL
HI 93740C-0	EDTA	2 packets
HI 93703-51	Dispersing Agent	4-6 drops (only when necessary, see note)

REAGENT SETS

HI 93740-01	Reagents (100 pcs of HI93740A-0, 100mL of HI93740B-0, 100 pcs of HI93740C-0, 20 mL of HI93703-51)
HI 93740-03	Reagents (300 pcs of HI93740A-0, 300mL of HI93740B-0, 300 pcs of HI93740C-0, 60 mL of HI93703-51)

DISPLAY CODE GUIDE

---	This indicates that the meter is in a ready state and zeroing can be performed.
5 IP	Sampling in Progress. This prompt appears each time the meter is performing a measurement.
-00-	This indicates that the meter is in a zeroed state and measurement can be performed.
2EAO	A zero reading was not taken. Insert a sample before adding reagent and press ZERO.
0.00	Under range. A blinking "0.00" indicates that the sample absorbs less light than the zero reference. Check the procedure and make sure you use the same cuvet for reference (zero) and measurement.
330	Over range. A flashing value higher than the maximum concentration readable (see specifications) indicates that the sample absorbs too much light, meaning that the concentration is too high. Dilute the sample.
CAP	Light over range. The cuvet is not inserted correctly and an excess ambient light is reaching the detector. If the cover is properly installed, then contact your dealer or the nearest Hanna Customer Service Center.
LO	Light under range. The zero sample is too dark for proper zeroing. If this is not the case, contact your dealer or the nearest Hanna Customer Service Center.
V 250	The "V" indicates that the battery voltage is getting low and the battery needs to be replaced.
-BA-	This indicates that the battery is dead and must be replaced. Note: once this indication is displayed, the meter will lockup. Change the battery to restart.

OPERATIONAL GUIDE


MEASUREMENT PROCEDURE

- Turn the meter on by pressing ON/OFF.



Note: for best results perform your tests between 20-24°C.

- When the LCD displays "- - -", it is ready.



- Fill one graduated beaker with 25 mL of deionized water (blank) and another one with 25 mL of sample.




- Add the content of one packet of HI 93740A phthalate-phosphate reagent to each beaker. Cap and shake gently until the reagent is dissolved.



Note: If sample contains iron (Fe^{3+}), it is important that all powder be dissolved completely before continuing with following step.


- Add 1 mL of HI 93740B 0.3% PAN solution to each beaker, swirl to mix and then wait for 15 minutes.




- Add one packet of HI 93740C EDTA reagent to each beaker, cap and swirl to mix until complete dissolution.



- Fill one cuvet up to 1.5 cm ($\frac{3}{4}$ ") below the rim with 10 mL of the blank.




- Place the cuvet into the holder and ensure that the notch on the cap is positioned securely into the groove.




- Press ZERO and "SIP" will appear on the display.



- Wait for a few seconds and the display will show "-0-". Now the meter is zeroed and ready for measurement.




- Fill a second cuvet up to 1.5 cm ($\frac{3}{4}$ ") below the rim with 10 mL of the reacted sample.



- Insert the second cuvet into the instrument.

- Press READ DIRECT and "SIP" will appear during measurement.



- The instrument directly displays concentration in mg/L of nickel on the Liquid Crystal Display.

Note: a temperature above 30°C may cause turbidity. In this case, before zeroing and taking readings, add 2-3 drops of Dispersing Agent (HI93703-51) to each cuvet and swirl until complete dissolution of turbidity.

INTERFERENCES

Interference may be caused by:

Co^{2+} must not be present

Fe^{2+} must not be present

Al^{3+} above 32 mg/L

Ca^{2+} above 1000 mg/L (as CaCO_3)

Cd^{2+} above 20 mg/L

Cl^- above 8000 mg/L

Cr^{3+} above 20 mg/L

Cr^{6+} above 40 mg/L

Cu^{2+} above 15 mg/L

F^- above 20 mg/L

Fe^{3+} above 10 mg/L

K^+ above 500 mg/L

Mg^{2+} above 400 mg/L

Mn^{2+} above 25 mg/L

Mo^{6+} above 60 mg/L

Na^+ above 5000 mg/L

Pb^{2+} above 20 mg/L

Zn^{2+} above 30 mg/L

TIPS FOR AN ACCURATE MEASUREMENT


The instruction listed below should be carefully followed during testing to ensure best accuracy.

- Do not touch the cuvet walls with hands.
- In order to maintain the same conditions during the zeroing and the measuring phases, it is necessary to close the cuvet to prevent any contamination.
- Do not let the test sample stand too long after reagent is added or accuracy will be lost.
- Whenever the cuvet is placed into the measurement cell, it must be completely free of fingerprints, oil or dirt. Wipe it thoroughly with HI 931318 or a lint-free cloth prior to insertion.
- It is important that the sample does not contain any debris. This would corrupt the readings.
- It is possible to take multiple readings in a row, but it is recommended that a zero reading be taken for each sample and that the same cuvet is used for zeroing and measurement.
- It is important to discard the sample immediately after the reading is taken because the glass might become permanently stained.
- Shaking the cuvet can generate bubbles in the sample, causing higher readings. To obtain accurate measurements, remove such bubbles by swirling or by gently tapping the vial.
- All the reaction times reported in this manual are referred to 20°C (68°F). As a general rule of thumb, they should be doubled at 10°C (50°F) and halved at 30°C (86°F).

BATTERY REPLACEMENT

Battery replacement must only take place in a non-hazardous area using a 9V alkaline battery.

Simply slide off the battery cover on the back of the meter. Detach the battery from the terminals and attach a fresh 9V battery while paying attention to the correct polarity. Replace the battery and the cover.



ACCESSORIES

REAGENT SETS

HI 93740-01 Reagents (100 pcs of HI93740A-0, 100mL of HI93740B-0, 100 pcs of HI93740C-0, 20 mL of HI93703-51)

HI 93740-03 Reagents (300 pcs of HI93740A-0, 300mL of HI93740B-0, 300 pcs of HI93740C-0, 60 mL of HI93703-51)

OTHER ACCESSORIES

HI 710009 Blue rubber boot

HI 710010 Orange rubber boot

HI 721310 9V battery (10 pcs)

HI 731318 Tissue for wiping cuvetts (4 pcs)

HI 731321 Glass cuvetts (4 pcs)

HI 731325 Caps for cuvetts (4 pcs)

HI 93703-50 Cuvets cleaning solution (230 mL).

CE DECLARATION OF CONFORMITY



DECLARATION OF CONFORMITY

We

Hanna Instruments Srl
V.le delle industrie 12
35010 Ronchi di Villafranca (PD)
ITALY

herewith certify that the colorimeters

HI93700 HI93701 HI93702 HI93704 HI93705 HI93706 HI93707
HI93708 HI93709 HI93710 HI93711 HI93712 HI93713 HI93714
HI93715 HI93716 HI93717 HI93718 HI93719 HI93720 HI93721
HI93722 HI93723 HI93724 HI93725 HI93726 HI93727 HI93728
HI93729 HI93730 HI93731 HI93732 HI93733 HI93734 HI93735
HI93736 HI93737 HI93738 HI93739 HI93740
HI93741 HI93742 HI93743 HI93744 HI93745 HI93746 HI93747
HI93748 HI93749 C101 C104

have been tested and found to be in compliance with the following regulations:

IEC 801-2 Electrostatic Discharge
IEC 801-3 RF Radiated
EN 55022 Radiated, Class B

Date of Issue: 19-02-1997

D.Volpato - Engineering Manager
On behalf of
Hanna Instruments S.r.l.

Recommendations for Users

Before using these products, make sure that they are entirely suitable for the environment in which they are used.

Operation of these instruments in residential area could cause unacceptable interferences to radio and TV equipments, requiring the operator to take all necessary steps to correct interferences.

Any variation introduced by the user to the supplied equipment may degrade the instruments' EMC performance.

To avoid damages or burns, do not perform any measurement in microwave ovens.