


Skincheck • Skincheck 1

HI 98109 • HI 98110 pH Testers for Skin

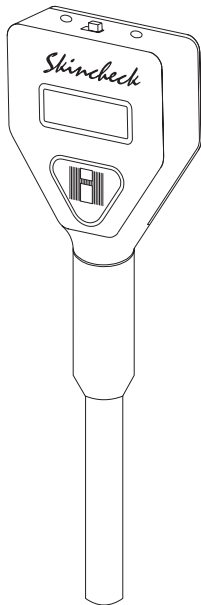

HANNA
instruments

www.hannainst.com

Dear Customer,
Thank you for choosing a Hanna product.
Please read carefully this instruction manual before using the instrument.
If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com.
These instruments are in compliance with the CE directives.

PRELIMINARY EXAMINATION

Remove the instrument from the packing material and examine it carefully to make sure that no damage has occurred during shipment. If there is any damage, immediately notify your Dealer.

Each meter is supplied complete with

- pH electrode:
 - HI 1413S/50 for HI 98109
 - HI 1413B/50 for HI 98110
- 2 x 1.5V alkaline batteries
- screwdriver and instructions


Note: Conserve all packing material until the instrument has been observed to function correctly. Any defective item must be returned in its original packing.

SPECIFICATIONS

Range	0.00 to 14.00 pH
Resolution	0.01 pH
Accuracy(@20°C)	±0.2 pH
Typical EMC Deviation	±0.1 pH
Calibration	Manual, 2 point
Electrode(included)	HI 1413S/50 for HI 98109 HI 1413B/50 for HI 98110
Environment	0 to 50°C (32 to 122°F); RH 95% max
Battery Type	2x1.5V alkaline
Battery Life	approx. 3000 hours of continuous use
Dimensions	66x50x25 mm (2.6x2.2x1") (meter only)
Weight	70 g (2.5 oz), HI 98109 90 g (3.2 oz.), HI 98110

ACCESSORIES

HI 1413B/50	Spare pH electrode with BNC connector and 1 m (3.3') cable for HI 98110
HI 1413S/50	Spare pH electrode with screw connector for HI 98109
HI 70004P	pH 4.01 buffer sachet (20 mL, 25 pcs)
HI 70007P	pH 7.01 buffer sachet (20 mL, 25 pcs)
HI 70010P	pH 10.01 buffer sachet (20 mL, 25 pcs)
HI 70300M	Storage solution, 230 mL bottle
HI 7061M	Cleaning solution, 230 mL bottle

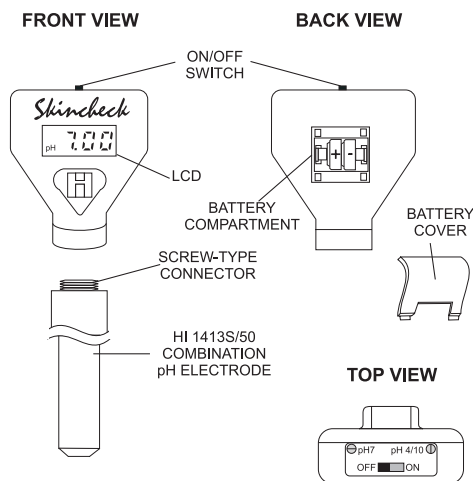

INITIAL PREPARATION

The pH electrode is shipped dry. Before using the meter, remove the protective cap and condition the electrode by soaking the tip (bottom 4 cm/1½") in pH 7.01 buffer solution for a couple of hours. Then follow the calibration procedure.

OPERATION

- Do not be alarmed if white crystals appear around the cap. This is normal with pH electrodes and they dissolve when rinsed with water.
- Connect the supplied electrode to the meter.
- Turn the tester on by sliding the switch on the top.
- Remove the protective cap and place the tip of the flat electrode on the surface to be measured (skin or scalp).

- For best results, wet the surface with distilled water or a neutral disinfectant.
 - After use, rinse the electrode with water and store it with a few drops of **HI 70300** storage solution in the protective cap.
- DO NOT USE DISTILLED OR DEIONIZED WATER FOR STORAGE PURPOSES.**
- Always replace the protective cap after use.

CALIBRATION


- For best results, calibrate frequently.
- Dip the tip of the electrode (4 cm/1½") in pH 7.01 buffer solution at room temperature. Allow the reading to stabilize.
- Use a small screwdriver to adjust the pH7 trimmer until the display reads "pH 7.01".
- Rinse the electrode with water and dip it in pH 4.01 (or pH 10.01) buffer solution. Allow the reading to stabilize.
- With a small screwdriver adjust the pH4/10 trimmer until the display reads "pH 4.01" (or "pH 10.01").
- Calibration is now complete.

ALWAYS CALIBRATE USING FRESH BUFFER SOLUTIONS.



BATTERY REPLACEMENT

Replace the batteries when the display fades or the meter cannot be switched on. Remove the battery cover on the back of the meter. Insert 2 new 1.5V batteries, while paying attention to their polarity.



Batteries should only be replaced in a safe area using the battery type specified in this instruction manual.

WARRANTY

These meters are **guaranteed for one year** against defects in workmanship and materials when used for its intended purpose and maintained according to instructions. **Electrodes are guaranteed for a period of six months.** This warranty is limited to repair or replacement free of charge. Damages due to accident, misuse, tampering or lack of prescribed maintenance are not covered. If service is required, contact the dealer from whom you purchased the instrument. If under warranty, report the model number, date of purchase, serial number and the nature of the failure. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the instrument is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization Number from the Customer Service department and then send it with shipment costs prepaid. When shipping any instrument, make sure it is properly packaged for complete protection.

Recommendations for Users

Before using this product, make sure that it is entirely suitable for the environment in which it is used. Operation of this instrument in residential areas could cause interference to radio and TV equipment. The glass bulb at the end of the pH electrode is sensitive to electrostatic discharges. Avoid touching this glass bulb at all times. Any variation introduced by the user to the supplied equipment may degrade the instrument's EMC performance. To avoid electrical shocks, do not use this instrument when voltage at the measurement surface exceeds 24 Vac or 60 Vdc. To avoid damage or burns, do not perform any measurement in microwave ovens.