

Instruction Manual

HI 38054 Ozone Test Kit



PEWA
Messtechnik GmbH

Weidenweg 21
58239 Schwerte

Tel.: 02304-96109-0
Fax: 02304-96109-88
E-Mail: info@pewa.de
Homepage: www.pewa.de

Dear Customer,

Thank you for choosing a Hanna Product.

Please read the instruction sheet carefully before using the test kit. It will provide you with the necessary information for correct use of the kit. If you need additional information, do not hesitate to e-mail us at tech@hannainst.com.

Remove the chemical test kit from the packing material and examine it carefully to make sure that no damage has occurred during shipping. If there is any noticeable damage, notify your Dealer or the nearest Hanna office immediately.

Each kit is supplied with:

- HI 93711-0 Total Chlorine Reagent, packets (100 pcs);
- Deionized Water, 1 bottle (500 mL);
- 1 checker disc (containing the 38054 disc);
- 2 glass vials with caps;
- 1 plastic pipette (3 mL).

Note: Any damaged or defective item must be returned in its original packing materials.

SPECIFICATIONS

Range	0 to 2.3 mg/L (ppm) as Ozone
Smallest Increment	0.1 mg/L
Analysis Method	Colorimetric
Sample Size	5 mL
Number of Tests	100
Case Dimensions	235x175x115 mm (9.2x6.9x4.5")
Shipping Weight	966 g (34.1 oz)

SIGNIFICANCE AND USE

Ozone is an oxidizing agent and a germicide. It is used for oxidation of organic matter, which produces color or odor in drinking water.

Note: mg/L is equivalent to ppm (parts per million).


CHEMICAL REACTION

The reaction between ozone and the reagent causes a pink tint in the sample which is proportional to the ozone concentration.


INSTRUCTIONS

READ THE ENTIRE INSTRUCTIONS BEFORE USING THE KIT


- Use the pipette to fill each glass vial with 5 mL of sample (up to the mark).
- Insert one of them into the left hand opening of the checker disc. This is the blank.

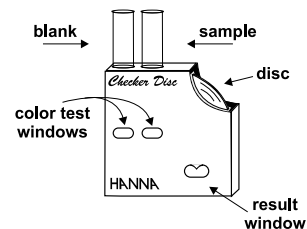

- Add to the other vial deionized water up to the 10 mL mark. Replace the cap and shake to mix.

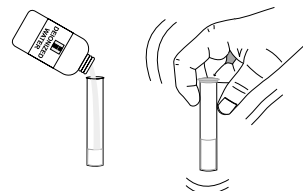


- Remove the cap and add 1 packet of HI 93711-0 reagent. Replace the cap and mix.




- Wait for 2 minutes to allow reaction to occur. This is the reacted sample.



- Remove the cap and insert the reacted sample into the right hand opening of the checker disc.
- Hold the checker disc so that a light source illuminates the samples from the back of the windows.



- Keep the checker disc at a distance of 30-40 cm (12-16") to match the color. Rotate the disc while looking at the color test windows and stop when you find the color match. Read the value in the result window directly in mg/L (or ppm) of Ozone.

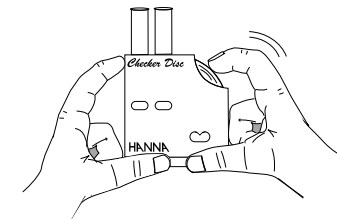

For best results: Perform the reading three times and take the average value (divide by 3 the sum of the three numbers). Intensely colored samples will make the color matching difficult and they should be adequately treated before performing the test. Suspended matter in large amounts should be removed by prior filtration.

Caution: Ultraviolet radiation may cause fading of colors. When not in use, keep the disc protected from light, in a cool and dry place.

Interferences: chlorine, bromine, iodine and oxidized manganese.

REFERENCES

Adaptation of the EPA recommended DPD method 330.5.

HEALTH AND SAFETY

The chemicals contained in this kit may be hazardous if improperly handled. Read the relevant Health and Safety Data Sheet before performing this test.